



Nitelog™ for Android

User Manual

For Use with Z1 Auto® CPAP machine



Thank you for choosing the Z1 Auto® CPAP System from Human Design Medical, LLC.

This *Nitelog for Android User Manual* provides information as to how to use the proprietary mobile app, *Nitelog*, to enhance your use of the Z1 Auto through its range of functionality from device remote control to data viewing available via its embedded *Bluetooth* capability. Please note all Z1 functions can be controlled without the use of this mobile app directly through the machine.

This *Nitelog for Android User Manual* is meant to supplement the information in the *Z1 Auto User Guide* that was provided with the purchase of the Z1 Auto CPAP. It is not intended to replace the *User Guide*. As such, the owner/user of the Z1 Auto System is responsible for reading and understanding the *User Guide*. The user is responsible for any injury or damage that results from:

- Operation of the Z1 other than in accordance with the operating instructions contained in the *User Guide* supplied.
- Unauthorized maintenance or modifications to the device or attached accessories.

Medical Information

Indications for Use

Your Z1 Auto System is a single patient, reusable device that provides continuous positive airway pressure (CPAP) to support treatment of adults weighing over 66 lbs (30 kg) with obstructive sleep apnea (OSA). Please see the *Z1 Auto User Guide* for Contraindications and Adverse Effects that may occur during the use of this medical device.

WARNINGS:

US Federal law restricts this device to sale by or on the order of a physician.

Use your Z1 and its accessories only for their intended use as described in the *User Guide* supplied with the Z1 Auto CPAP and as directed by your physician, clinician or healthcare provider.

Data

All data generated through *Nitelog* will be stored solely on your Android device. HDM will not receive, store or back-up any of your data and is not responsible for any loss of your data. Please review the privacy policy on HDM's website before using *Nitelog*.

Because access to your data and the ability to control your Z1 Auto are protected by the password that you create using the *Nitelog* app and the passwords that secure your Android device generally, we highly recommend that you do not share your passwords with other people. In addition, because the password on your Z1 Auto may be reset by any person in physical possession of your Z1 Auto, we highly recommend that you maintain physical security over your Z1 Auto device to avoid unauthorized access to and control of the settings and data on your Z1 Auto.





Quick Start

1. Make sure the Z1 Auto is plugged in and sitting next to the Android device.
2. Make sure that **Bluetooth** is enabled in your phone settings and the Z1.
3. To **connect to a Z1**, click the '+' button in Nitelog, open Device List, and select your device.
4. Set your Z1 password (see page 4).
5. Once connected, the Nitelog main screen (Classic View (see page 5)) will light up and **display live Z1 information** as it updates.
6. Use the start/stop button on Classic View just as you would on the Z1 to start and stop the Z1.
7. View and edit **Z1 device settings** by swiping left on the Classic View. (page 5)
8. **View your data** with Chart View (see page 6) by clicking the top middle icon on the main screen.
9. To **update your sleep data**, use the green sync button located at the bottom of Chart View. (page 6)
10. **Share your data or generate compliance reports** by clicking the action menu on the bottom left of Chart View. (page 5–7)
11. View **more options** by clicking the gear icon in the top right corner of the Classic View. (page 9-10)


Set Password

1. To change or set your password, press "Update Password" on the initial password screen. After choosing "Update Password", the screen below will appear.
2. Type in your new password in the first field and then type in your new password a second time in the "Verify Password" field. Save.
3. Press and hold the power button on the Z1 for two seconds to confirm the password change. You will have 20 seconds to confirm.
4. If your password has been saved successfully, the below picture will be displayed.
5. The password may fail for the following reasons:
 - User cancels the change
 - Z1 has timed out
 - Z1 is not in Standby Mode


To reset password, check that your Z1 is in Standby mode, close the failure screen, and repeat steps 1–4.

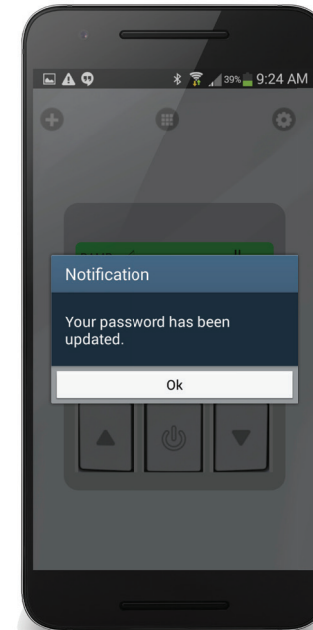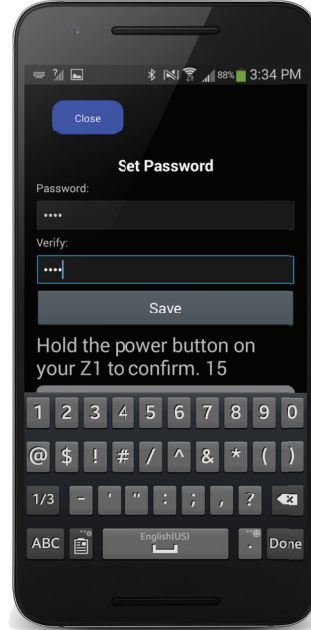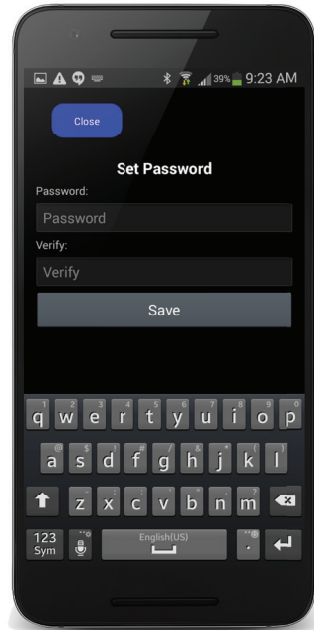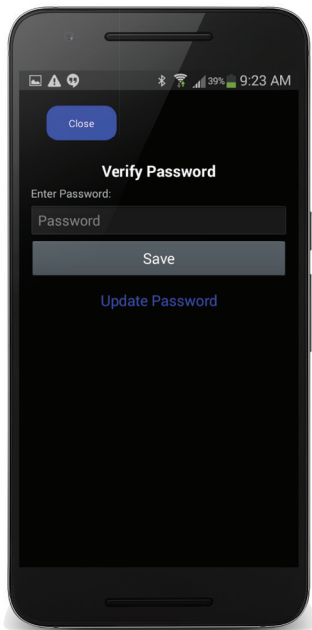

If you want to reset the password after you are logged in, open Options on the main screen and click the gear in the upper right. Press "Set Password" to set a new password.

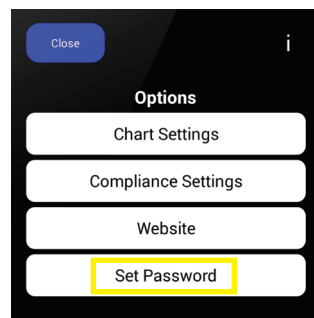

Classic View

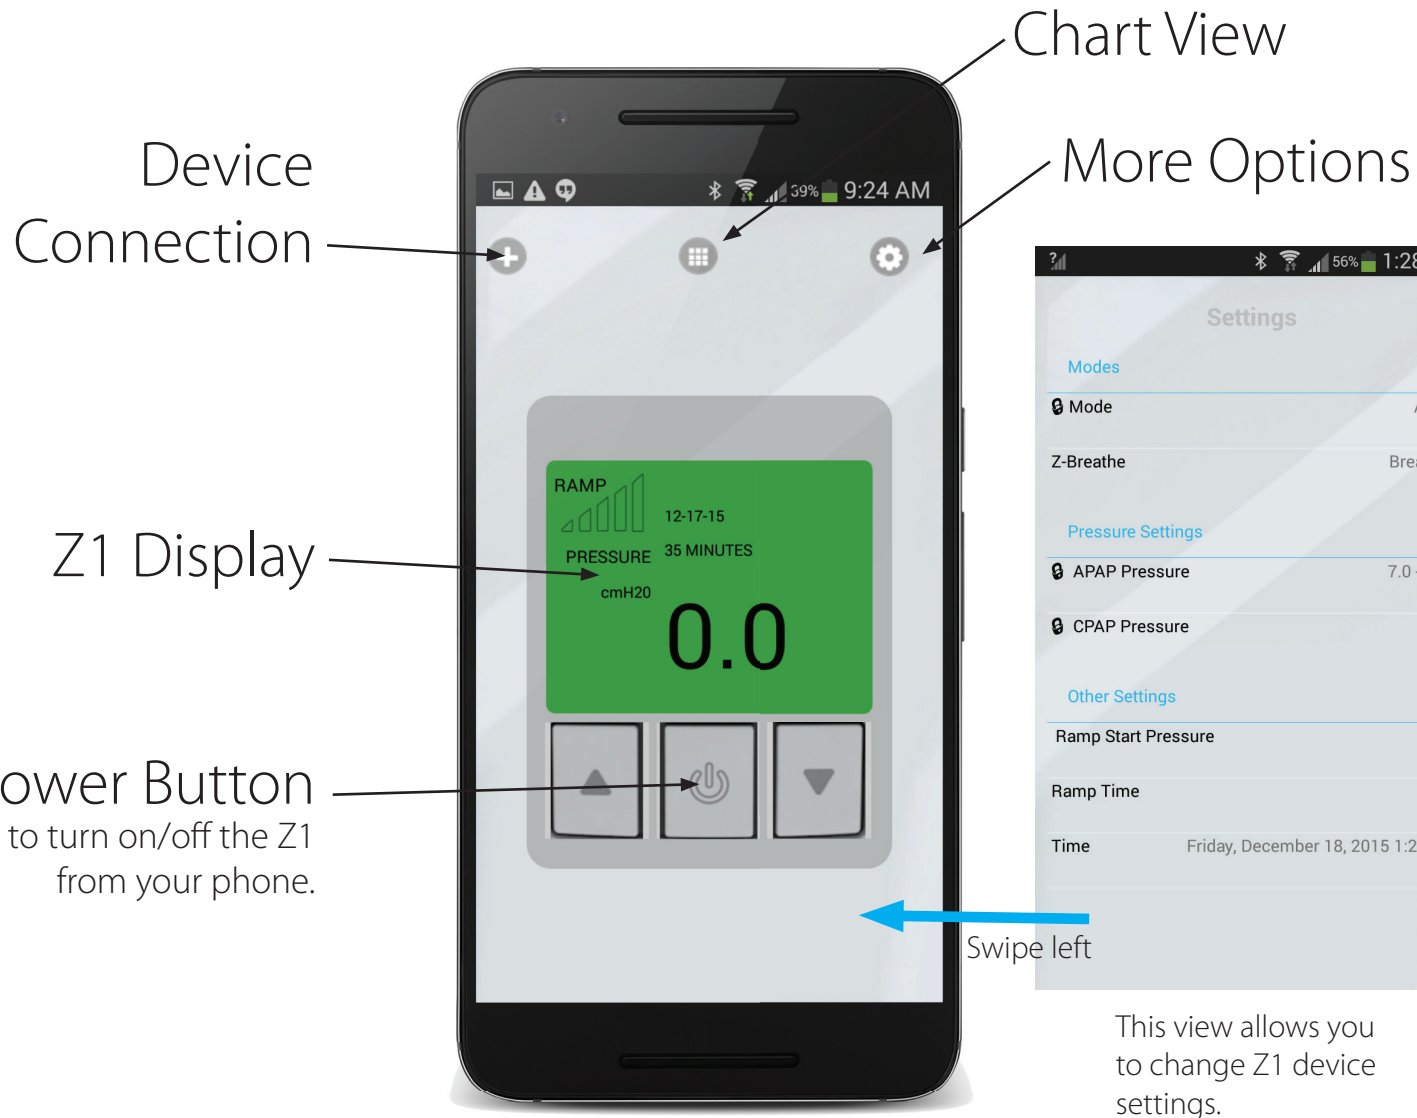

This lock symbol means you may access only your Z-Breathe™, Ramp Start Pressure, Ramp Time and Device Date + Time settings. For Mode, CPAP Pressure and APAP Pressure settings please contact your Healthcare Provider if changes are desired.

Chart View


Press these three buttons to select which chart to display below (AH Count, Usage Hrs, or AH Index/Pressure). The selected button is highlighted.

Chart

View charts in portrait or landscape by rotating your device.

Action Menu

This menu gives you options for sharing your data and generating reports.

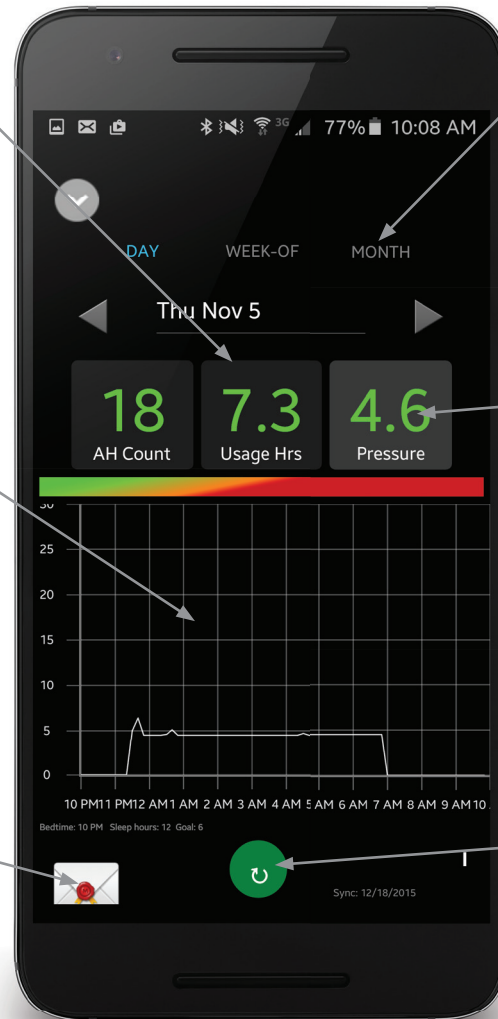

Navigation

Navigate your data using the arrows, or by swiping, pinching or zooming.

Pressure / AH Index Toggle


Press this button to toggle between Pressure and AHI


Sync

Use sync to get sleep data from your Z1.

Share Your Data


Sending

1. Press the action menu. 
2. Select the share option.
3. A new email draft will be created that includes your data.
4. "Screenshot" will save a chart snapshot to Photos which can be sent via text message or email.

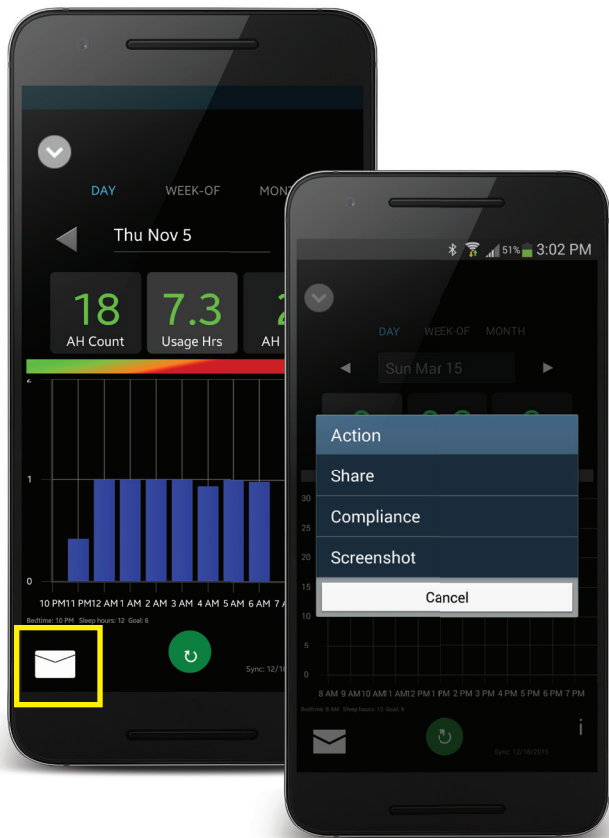

Receiving



1. A Nitelog user can click and hold the attached file from their phone to open in the app.
2. Non-Nitelog users can view a screenshot of data.

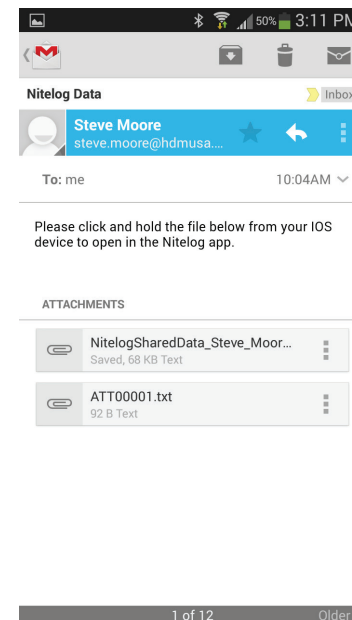

*The blue bar at the top of Chart View indicates that shared data is being viewed. To exit this mode, close Chart View and click the option to stop viewing shared data when prompted.

Generate Compliance Reports

1. To generate a compliance report, select the compliance option from the action menu.
2. Modify how a report is generated using Compliance Settings. (see page 11)

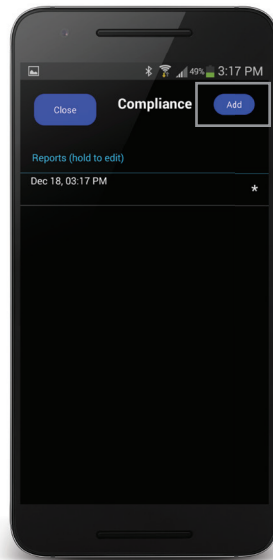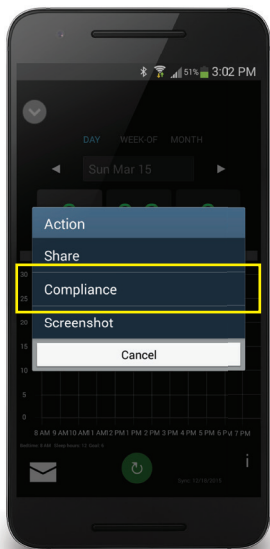

Patient: Anonymous
12/18/2015 3:17 PM



Compliance Report

PARAMETERS

Range: 3 months(12/15/2014 8:00 AM-3/15/2015 8:00 AM)
Window: 30 days
Days Required: 21
Hours Required: 4

Details for Compliance Window

12/15/2014 8:00 AM-3/15/2015 8:00 AM

Total Days: 90
Days Used: 1.0
Hours Used: 0.2166667

Days Used \geq Required Hours: 0.0
Days Used $<$ Required Hours: 90.0
% Days Used \geq Required Hours: 0.00

Avg Daily Usage From Days Used: 0.22
Avg Daily Usage From Total Days: 0.00

Compliance Met: false

Manage Users and Devices

Devices

1. Make sure that Bluetooth is enabled in your phone settings and the Z1.
2. Connect to a device by selecting from the list.
3. Disconnect from devices using the Disconnect button.





Adding your Name to the Compliance Data




1. Make sure that Bluetooth is enabled in your phone settings and the Z1.
2. Press the Users: Anonymous button
3. Press the Manage button
4. On the Legal Disclaimer Page, slide OFF to ON
5. Press First Name and Last Name and type in your name.



Chart Settings

1. Locate Chart Settings in the option menu. 
2. Use the sliders under AH Threshold to set the green and red zones in the AH Index chart and Q-Bar, representing good and bad sleep quality.
3. The Q-Bar shows total sleep time versus goal and the proportions of good, Ok and bad quality sleep.






-  Good– ideal / optimal
-  OK – acceptable
-  Bad – poor



Compliance Settings

1. Compliance Settings are the parameters used to determine whether or not compliance has been achieved.
2. Open Compliance Settings from the Option menu.
3. Generate a report by clicking the action button in Chart View.

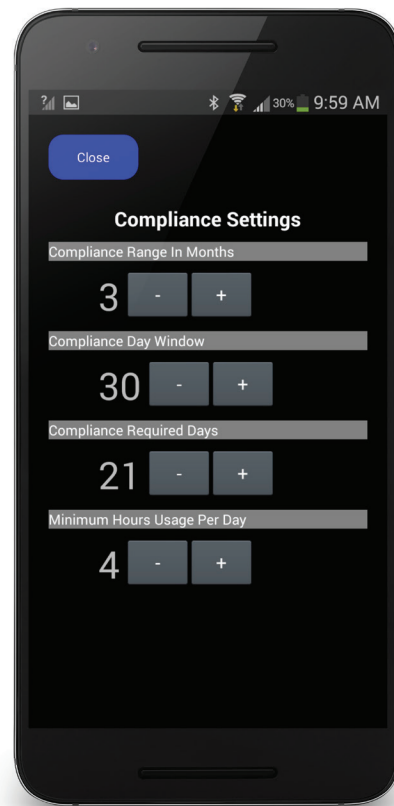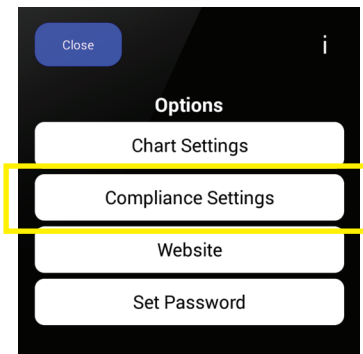

 Patient: John Doe
12/21/2015 11:04 AM

Compliance Report

PARAMETERS

Range: 3 months(8/3/2015 10:00 PM-11/1/2015 10:00 PM)
Window: 30 days
Days Required: 21
Hours Required: 4

Details for Compliance Window

8/3/2015 10:00 PM-11/1/2015 10:00 PM

Total Days: 90
Days Used: 4.0
Hours Used: 24.68333

Days Used ≥ Required Hours: 4.0
Days Used < Required Hours: 86.0
% Days Used ≥ Required Hours: 1.00

Avg Daily Usage From Days Used: 6.17
Avg Daily Usage From Total Days: 0.27

Compliance Met: false

Troubleshooting

- I don't see all of my data.
 1. Make sure the date and time matches on the device and in Z1 Settings.
 2. Check Chart Settings to make sure the sleep time and duration are within the viewable range.
 3. Click the Sync button.
 4. Verify that you have selected the correct date and day, week, or month range.
- I don't see my device in the Device List.
 1. Make sure that Bluetooth is enabled on your phone and the Z1.
 2. Unplug your Z1 for five seconds, plug it back in, and open Device Settings.
- I can't swipe to Device Settings.
 1. Make sure you are connected to your device.
 2. Make sure you are swiping left.
- I don't know my password.
 1. Try to connect to your device, then use the Update Password option.
- I have another issue.
 1. Try restarting the app by double clicking the home button, closing and re-opening Nitelog.
 - * To close the app, double click the home button, then swipe up the Nightlog screenshot.
 2. Please send us a report by going to the option menu and selecting the report option. This will create an email that goes to Z1MobileFeedback@hdmusa.com.
 3. For more troubleshooting tips and support, use the app and click the website button in the Option View.





Nitelog™

As of the release date on December 21, 2015 the following Android devices have been tested

Device	OS build	Result
Samsung Galaxy S3	Android 4.4.2	PASS
Samsung Galaxy S4	Android 4.4.2	PASS
Samsung Galaxy S5	Android 5.0	PASS
Samsung Galaxy S6	Android 5.1.1	PASS
Samsung Galaxy Note 5	Android 5.1.1	PASS
HTC One M8	Android 4.4.2	PASS
Motorola Moto G2 (2nd gen)	Android 5.0.2	PASS
LG Nexus 5	Android 4.4.2	PASS
Sony Xperia Z3	Android 4.4.4	PASS
Lenovo Yoga Tablet 10 HD+	Android 4.3	PASS

Human Design Medical, LLC
Charlottesville, VA 22902

Main phone (Supplies & replacement parts): 1-855-436-8724 [1-855-HDMUSA4]
Service support or warranty coverage: 1-855-436-8729 [1-855-HDMUSA9]

Email: service.support@hdmusa.com

40-0059 Rev A, User Manual, Z1 Mobile App, Android v1 122115

Nitelog™ is a trademark of Human Design Medical, LLC. Z1 Auto®, The HDM logo (HDM logo icon), Z1®, and Z-Breathe® are registered trademarks of Human Design Medical, LLC. Breas is a registered trademark of Breas Medical AB. All other trademarks are the property of their respective owners.

