

**PHILIPS**

DreamStation 2

Auto CPAP Advanced



**Respshop**  
better sleep, better life.

Introducing  
**DreamStation 2**  
**Auto CPAP Advanced**  
Success. By design.




# Evolving to a new way of doing business

The business of treating patients for obstructive sleep apnea (OSA) can seem complex. Recent changes to our daily lives will become the standard moving forward.

**Philips DreamStation 2 Auto CPAP Advanced**, our next clinically proven<sup>1</sup> evolution in integrated sleep therapy solutions, is designed to help you succeed by supporting you to treat patients effectively and efficiently across the OSA journey.

Improvements include simplified setup and training as well as new features designed to increase comfort, drive adherence and enhance efficiencies in patient management.

## The OSA Journey

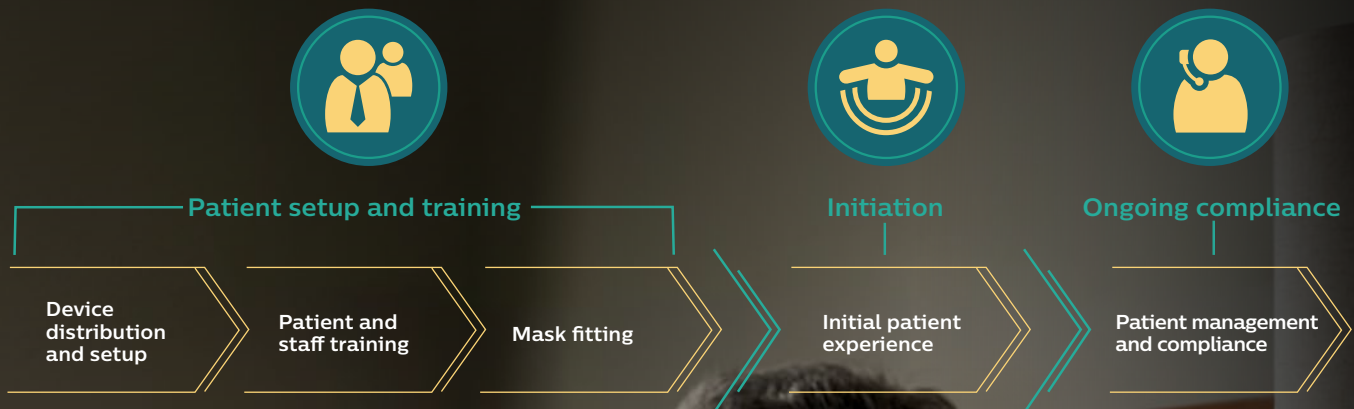

# Philips DreamStation 2 Auto CPAP Advanced Success. By design.

Simplified.  
Intuitive.  
Connected.



DreamStation 2 Auto CPAP Advanced is designed to help you and your patients succeed...together.




## Patient setup and training

**Efficient setup:** Flexibility in the setup process allows you to choose what is best for your business.

1. Out-of-the-box, no-touch setup<sup>2</sup>
  - Accept data-driven defaults
  - Personalize remotely with Care Orchestrator
2. Streamlined, low-touch, first-ever guided setup on the device

**Simplified training:** The CPAP features intuitive navigation of comfort features and settings, along with easy handling of the device.

**Precision mask fitting:** Philips Respironics Mask Selector uses no-touch scanning technology for the right mask fit from the start.<sup>3</sup>



RTs set up **DreamStation 2 Auto CPAP Advanced** 28.7% faster than DreamStation on first try.<sup>4</sup>

To learn more, visit [philips.com/dreamstation-2](https://philips.com/dreamstation-2)



## Initiation

**Three easy-to-access comfort settings:** Live adjustments of Ramp Plus, humidification and heated tube temperature while therapy is running are included.

- Ramp Plus allows patients to set a comfortable starting pressure for falling asleep, which may also help reduce callbacks and adjustments to minimum pressure prescriptions.

**Micro-flexible 12mm heated tube:** Philips smallest-diameter tubing is designed to be comfortable while taking up less space than traditional tubing.

**Smart auto and advanced algorithms:** Proprietary algorithms automatically adjust pressure to provide personalized therapy and treat AHIs at lower pressures.<sup>5</sup>



## Ongoing compliance

**Enhanced connectivity:** Integrated cell modem with automatic Bluetooth pairing enables remote setup and easy access to data for both your care team and your patients.

- On-demand prescription changes
- Remote troubleshooting through Performance Check

**Philips Care Orchestrator:** Drive collaboration among your team with patient insights delivered straight to smartphones, tablets or PCs.

- Adherence Profiler enables you to get notifications if a patient is at risk of noncompliance in a 90-day period.



**DreamMapper app** keeps patients engaged with easy access to coaching to drive ongoing compliance.

Patients struggling with adherence to sleep therapy have a **283% higher success rate**.<sup>6</sup>

# Introducing DreamStation 2 Auto CPAP Advanced



22% smaller

than a leading competitor

29% smaller than  
DreamStation<sup>1</sup>

16% lighter

than a leading competitor

2.5% lighter than DreamStation<sup>1</sup>  
(with power supply included)<sup>1</sup>

## Device components



Water tank  
with lid



Reusable  
pollen filter



Ultrafine  
pollen filter

# Ordering information

## DreamStation 2 Auto CPAP Advanced part numbers

PN	PN description
DSX520H11C	DreamStation 2 Auto CPAP Advanced + Humidifier with cell/BT
DSX520T11C	DreamStation 2 Auto CPAP Advanced + Humidifier/Heated Tube with cell/BT

## DreamStation 2 accessories

PN	PN description
1146072	DS2 Humidifier Water Tank no Lid, RP
1146073	DS2 Humidifier Lid only, RP
1142836	DS2 Inlet/Outlet Seal, RP
1142832	DS2 Water Tank with Lid
1142687	DS2 Reusable Pollen Filter, RP
1142828	DS2 Disposable Ultra-Fine Filter, RP
1142829	DS2 Disposable Ultra-Fine Filter, RP
1142831	DS2 Disposable Ultra-Fine Filter, RP
1144877	3150 BLE Wrist Ox
1147077	Soft Reusable Finger Sensor, WristOx, SM
1147178	Soft Reusable Finger Sensor, WristOx, M
1147179	Soft Reusable Finger Sensor, WristOx, L
1147180	PC USB Interface Cable, WristOx 3150 BLE
1142834	DS2 Carrying Case
1145156	DreamStation 2 Roll Stand

## DreamStation/ DreamStation 2 Auto CPAP Advanced accessories

PN	PN description
HT15	15 mm Heated Tube
PR15	15 mm Standard Tube
PR12	12 mm Micro-Flexible Tube
HT12	12 mm Micro-Flexible Heated Tube
1032907	22 mm Performance Tube
1147466	12 mm Tube Device Adapter with OIS
1145085	Philips RI SD Card, 1 pack
1063859	Philips RI SD Cards, 10 pack
1120746	EN: Shielded DC Cord - DreamStation
1120747	EN: Shielded DC Cord System - DreamStation
1144267	Philips 80W CPAP Power Supply
1005894	Power Cord with C7 END-USA/CAN
532209	DC Battery Adapter Cable
1124009	PAP Lithium Ion Battery Kit
1121736	Lithium Ion Battery, PAP Device Cable
1126947	Lithium Ion Battery Case
342077	Bacteria Filter
302418	Pressure Valve
312710	O <sub>2</sub> Enrichment Attachment

**References:** **1.** Gagnadoux F, Pevernagie D, Jennum P, Lon N, Loiodice C, Tamisier R, van Mierlo P, Trzepizur W, Neddermann M, Machleit A, Jasko J, Pépin JL. Validation of the System One RemStar Auto A-Flex for Obstructive Sleep Apnea Treatment and Detection of Residual Apnea-Hypopnea Index: A European Randomized Trial. *J Clin Sleep Med.* 2017 Feb 15;13(2):283-290. doi: 10.5664/jcsm.6464. PMID: 27784415; PMCID: PMC5263084. Kushida CA, Berry RB, Blau A, Crabtree T, Fietze I, Kryger MH, Kuna ST, Pegram GV Jr, Penzel T. Positive airway pressure initiation: a randomized controlled trial to assess the impact of therapy mode and titration process on efficacy, adherence, and outcomes. *Sleep.* 2011 Aug 1;34(8):1083-92. doi: 10.5665/SLEEP.1166. PMID: 21804670; PMCID: PMC3138163. **2.** Assumes acceptance of smart, default settings. Alternatively, you can set up prescriptions entirely via CO with no device touch. **3.** Data analysis after 90 days of use. 2019 Philips sponsored patient preference trial (n=310). Patient scanned using the Mask Selector (n=153) vs. Traditional fitting methods (n=157). **4.** Philips randomized usability trial. Ease-of-Set Up and Time-to-Set Up of Continuous Positive Airway Pressure (CPAP) Devices; evaluating the user interface with 27 respiratory therapists that typically set up Philips DreamStation and ResMed AirSense 10 CPAP devices. 2020. **5.** Hertegonne KB, Rombaut B, Houtmeyers P, Van Maele G, Pevernagie DA. Titration efficacy of two auto-adjustable continuous positive airway pressure devices using different flow limitation-based algorithms. *Respiration.* 2008;75(1):48-54. doi: 10.1159/000103515. Epub 2007 Jun 1. PMID: 17541262. Nolan GM, Ryan S, O'Connor TM, McNicholas WT. Comparison of three auto-adjusting positive pressure devices in patients with sleep apnoea. *Eur Respir J.* 2006 Jul;28(1):159-64. doi: 10.1183/09031936.06.00127205. Epub 2006 Mar 29. PMID: 16571610 Nieves Navarro Soriano, Mikel Azpiazu Blocona, Javier Carrillo Hernández-Rubio, Raquel Cobos Campos, Ainhoa Alvarez Ruiz de Larrinaga, Berenici Murià Diaz David Diez Fuente, Carlos Javier Egea Santaolalla. The Effective Pressure of the CPAP Titration Depends on the APAP Device Used. Poster at SEPAR Convention (Spain). May 2018. Javier Carrillo Hernandez-Rubio, Mikel Azpiazu Blocona, David Diez Fuente, Nieves Berlen Navarro Soriano, Laura Cancelo Diaz, Lourdes Guerra Martin, Raquel Cobos Campos, Carlos Javier Egea Santaolalla. Validity of the CPAP Automatic Titration in our Sleep Unit. Poster at SEPAR Convention (Spain). May 2018. **6.** 46% of DreamMapper patients went on to achieve adequate adherence within 90 days versus 12% for the Standard Care group, a relative increase of 283.33%. In a retrospective review conducted by Philips Respiroics of the EncoreAnywhere database (white paper) of struggling patients (n=24,176).

Caution: Federal law restricts this device to sale by or on the order of a physician.

©2021 Koninklijke Philips N.V. All rights reserved. Specifications are subject to change without notice. Trademarks are the property of Koninklijke Philips N.V. or their respective owners.



philips.com/dreamstation-2  
edoc JB 2/11/21 MCI 4110705 v00

1010 Murry Ridge Lane, Murrysville, PA 15668  
800 313 0984